BAYER

Contour® next link

Wireless Blood Glucose
Monitoring System

NO CODING™

Medtronic

Uses only CONTOUR®NEXT blood glucose test strips from Bayer

USER GUIDE

INTENDED USE

The CONTOUR®NEXT LINK wireless blood glucose monitoring system from Bayer (meter, test strips and control solution) is intended for self-testing by persons with diabetes to monitor glucose concentrations for the quantitative measurement of glucose in fresh capillary whole blood drawn from the fingertip or palm. **It is intended for *in vitro* diagnostic use only**. The clinical utility of this device is that it may be used as an aid to monitor the effectiveness of a diabetes control program.

The CONTOUR NEXT LINK wireless blood glucose monitoring system is intended to be used to transmit glucose values to Medtronic devices and facilitate transfer of information to Medtronic CareLink® Software through use of radio frequency communication.

The CONTOUR NEXT LINK wireless blood glucose monitoring system from Bayer is not intended for the diagnosis of or screening for diabetes mellitus and it is not intended for use on neonates.

IMPORTANT SAFETY INFORMATION

⚠️ **WARNINGS**

Serious Illness

- Capillary (fingerstick or Alternative Site) blood glucose testing may not be clinically appropriate when peripheral flow is decreased. Shock, severe hypotension, hyperosmolar hyperglycaemia, diabetic ketoacidosis and occurrence of severe dehydration are examples of clinical conditions that may adversely affect the measurement of glucose in peripheral blood.[1-3]
- Keep out of reach of children. This kit contains small parts which could cause suffocation if accidentally swallowed.

Talk to Your Health Care Professional

- Before setting any Target ranges or High or Low Alerts on your meter.
- Before changing your medication based on test results.
- If your blood sugar reading is under 2.8 mmol/L, follow medical advice immediately.
- If your blood sugar reading is over 13.9 mmol/L, wash and dry your hands well and repeat the test with a new strip. If you get a similar result, call your health care professional as soon as possible.
- About whether Alternative Site Testing (AST) is appropriate for you.

Potential Biohazard

- Always wash and dry your hands well with soap and water before and after testing, handling the meter, lancing device or test strips.
- The lancing device and lancets are for single person use. Do not share them with anyone including other family members. Do not use on multiple persons.[4,5]
- All parts of this kit are considered biohazardous and can potentially transmit infectious diseases, even after you have performed cleaning. For cleaning instructions, please see Cleaning Your Meter, page 66.
- The MICROLET®2 lancing device is intended for self-testing by a single patient. It must not be used on more than one person due to the risk of infection.
- ⊗ Use a new MICROLET® lancet each time you test because it is no longer sterile after use.
- Always dispose of test strips and lancets as medical waste or as advised by your health care professional. All products that come in contact with human blood should be handled as if capable of transmitting infectious diseases.

PRECAUTIONS

- Read your CONTOUR®NEXT LINK user guide, the MICROLET®2 lancing device package insert, your Medtronic device user guide and all instructional materials provided in your meter kit before testing. Please follow all instructions for use and care exactly as described to help avoid inaccurate results.
- Examine product for missing, damaged or broken parts. If the test strip bottle is open inside a new box of strips, do not use those strips. For replacement parts, contact Bayer Diabetes Support. Please see back cover for contact information.
- The CONTOUR NEXT LINK meter from Bayer only works with CONTOUR®NEXT test strips and CONTOUR®NEXT control solutions.
- Always keep the CONTOUR NEXT test strips in their original bottle. Tightly close the bottle immediately after removing a test strip. The bottle is designed to keep the test strips dry. Avoid exposing meter and test strips to excessive humidity, heat, cold, dust and dirt. Exposure to room humidity from leaving the bottle open or not storing the strips in their original bottle can damage your test strips. This could lead to inaccurate results. Do not use a test strip that appears damaged or has been used.
- Check the expiry dates on your test strips and control solution. Do not use the test strips or control solution if the expiry date printed on the bottle label and carton has passed. This can cause inaccurate results. For the control solution, do not use if it has been 6 months since you first opened the bottle. After first opening the bottle, write the 6-month discard date on the control solution label.
- If your control solution test result is out of range, contact Bayer Diabetes Support. Please see back cover for contact information. Do not use the meter for blood glucose testing until you resolve this issue.
- The meter has been designed to give accurate results at temperatures between 5° to 45°C. If you are outside this range, you should not test. Whenever the meter is moved from one location to another, allow approximately 20 minutes for the meter to adjust to the temperature of the new location before performing a blood glucose test.
- Do not perform a blood glucose test when the CONTOUR NEXT LINK meter is connected to a computer.

- Use only approved cables or wall charger from the manufacturer or a 5V charger that displays a CE mark.
- Your CONTOUR®NEXT LINK meter from Bayer has been preset and locked to display results in mmol/L (millimoles of glucose per litre of blood).
  - ❖ Results in mmol/L will **always** have a decimal point.
  - ❖ Results in mg/dL will **never** have a decimal point;

    Example: $5.2^{\frac{mmol}{L}}$ or $93^{\frac{mg}{dL}}$

  - ❖ Check your display screen to make sure the results are shown the right way. If not, please see Bayer Diabetes Support contact information on the back cover of this user guide.
- The CONTOUR NEXT LINK wireless blood glucose monitoring system from Bayer has a measuring range of 1.1 mmol/L to 33.3 mmol/L.
  - ❖ For results under 1.1 mmol/L or over 33.3 mmol/L:
    - ○ If your blood sugar reading is under 1.1 mmol/L, the "Follow Medical Advice Immediately" screen will display and the meter will beep twice. Contact your health care professional.
    - ○ If your blood sugar reading is over 33.3 mmol/L the next screen will tell you to retest. The meter will beep twice. If results are still over 33.3 mmol/L, "Follow Medical Advice Immediately" is displayed.
- Please be aware that USB ports in some computers and self-powered USB hubs can become much warmer than the room. A USB extension cable is available. If you wish to test immediately after disconnecting from your computer, please use the USB cable to protect the meter from exposure to heat created by the computer.

CAUTION: Your CONTOUR NEXT LINK meter only works with CONTOUR®NEXT test strips and CONTOUR®NEXT control solutions.

Rechargeable Battery

Your CONTOUR®NEXT LINK meter from Bayer has a rechargeable battery. You must charge your battery before you can use your meter and you cannot do a blood sugar test while the battery is charging.

Charge Your Meter Using a Wall Outlet or a Computer

- Remove USB cap.
- Insert the meter USB plug into the wall charger* or use the USB extension cable.

The meter is fully charged when the test strip port light stops flashing and turns off.

*Charger is available separately from Bayer Diabetes Support if not included in your meter kit. See contact information for Bayer Diabetes Support on back cover.

> **CAUTION:** Do not perform a blood glucose test when your meter is connected to an external device, e.g., computer.

NOTE: Your meter can Rapid Charge. After 1 minute of charging, you can unplug the meter and run one blood sugar test, if needed.

A USB extension cable is included for your convenience.

OR
- Remove USB cap.
- Insert the meter USB plug into your computer or use the USB extension cable.
- Be sure your computer is turned on and not in sleep, hibernate or power save mode.

> **CAUTION:** Please be aware that USB ports in some computers and self-powered USB hubs can become much warmer than the room. If you wish to test immediately after disconnecting from your computer, please use the USB cable to protect the meter from exposure to heat created by the computer.

vi

Table of Contents

GETTING STARTED

TESTING

FEATURES

USING THE MAIN MENU

TECHNICAL INFORMATION AND CARE

Getting Started

The CONTOUR®NEXT LINK Wireless Blood Glucose Monitoring System from Bayer

The CONTOUR NEXT LINK wireless blood glucose monitoring system from Bayer only works with CONTOUR®NEXT test strips from Bayer.

Top Menu Button
See page 4

Display Screen

Meter USB Plug

12:00 | 13.10
5.2 mmol L
Before Meal

Reminder
Notes

Test Strip Port
Insert the test strip here. To turn on the test strip port light, see page 4.

Selection/Scrolling Buttons
See page 4

Protective USB Cap
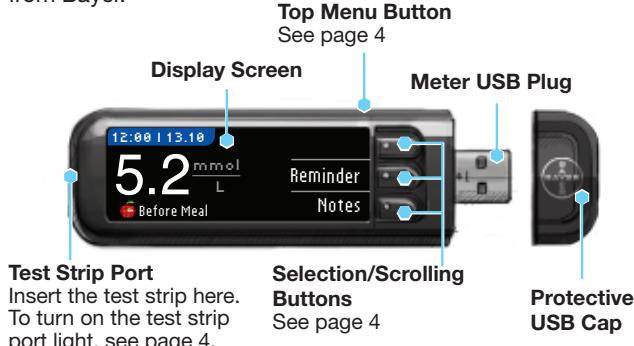
> ⚠️ **WARNING**
> **Keep out of reach of children. Accidental swallowing could cause suffocation.**

Your CONTOUR NEXT Test Strip

Grey Square End
Insert this end into the test strip port with the grey end facing up.
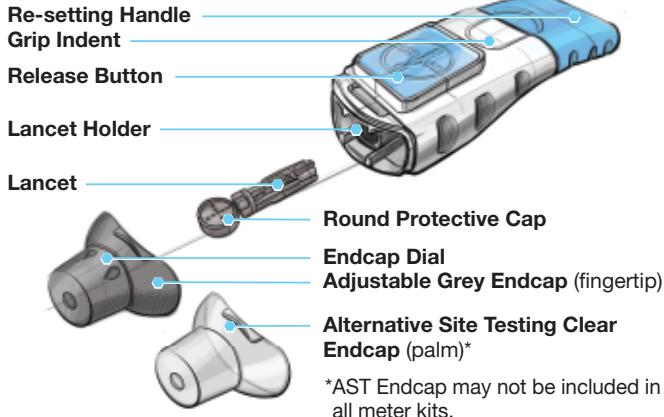
Sample Tip
Blood sample pulled in here.

> **CAUTION:** The CONTOUR NEXT LINK meter from Bayer only works with CONTOUR NEXT test strips and CONTOUR®NEXT control solutions.

Contour next link

Your MICROLET®2 Lancing Device

Re-setting Handle
Grip Indent

Release Button

Lancet Holder

Lancet

Round Protective Cap

Endcap Dial
Adjustable Grey Endcap (fingertip)

Alternative Site Testing Clear Endcap (palm)*

*AST Endcap may not be included in all meter kits.

"Talks" to Your Compatible Medtronic Device

Your CONTOUR®NEXT LINK meter can automatically send your blood glucose result directly to your compatible Medtronic device, if your meter and pump are linked. This eliminates the need to manually enter your blood glucose result into your insulin pump. Your compatible Medtronic device will only accept the glucose result if the Meter Send Option in your device's Utility Menu is set to On and you have programmed the device with the meter's ID (serial) number. Up to 3 CONTOUR NEXT LINK meters can be connected to your Medtronic pump. To use the meter link features, your CONTOUR NEXT LINK meter and Medtronic device must be within 1.22 meters (4 feet) of each other. If you are not using the meter link feature, you may want to set the Send Option to Never on your CONTOUR NEXT LINK meter to save battery power.

Meter Overview

Turning the Meter On or Off

• Press and hold the top **Menu** button to turn the meter on or off.

• Insert a test strip to turn the meter on.

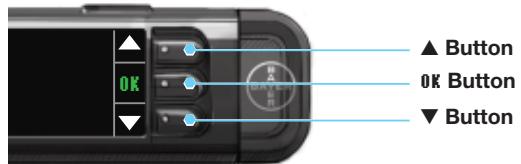• Meter turns off after 3 minutes of inactivity.

Using the Top Menu Button

The top **Menu** button has three functions:

• **To turn the meter on/off**, press and hold the top **Menu** button.

• **To go back one screen** from most screens, press the top **Menu** button once.

• **To turn on/off the test strip port light**, quickly press the top **Menu** button twice.

Using the Selection/Scrolling Buttons

▲ **Button**

OK Button

▼ **Button**

• The three buttons next to the screen allow you to make your selection by pressing the button next to your choice.

• Scroll up or down for additional choices when the ▲ or ▼ arrows appear on the meter screen.

4

• When your choice is highlighted, make a selection by pressing **OK**.

NOTE: Press and hold the ▲ or ▼ button to scroll through the list faster.

Using the Main Menu

Logbook
Trends
Setup

The Main Menu has three choices: Logbook, Trends and Setup. Select one by pressing the button next to your choice.

CAUTION: Unplug meter from charging source before beginning Setup.

Initial Setup

1. **Before use, fully charge your meter. See page vi.**

Turn On

2. Press and hold the top **Menu** button until the meter turns on. After a welcome screen, you see the **Language** choice screen.

5

Set Language

LANGUAGE
✔ English
Deutsch
Español
OK ▼

3. Press the ▼ button to see more language choices. When your language is highlighted, press **OK**.

✔ Language:
English
✔ OK
✗ No

4. Press **OK** to confirm.

If the correct language is not displayed, press **No**.

Connect to Pump

CONNECT TO PUMP ❓
Connect to a MiniMed
Pump?
OK
Skip

5. If you are connecting to a MiniMed pump now, press **OK** and go to Step 6. If not, press **SKIP** and go to Step 17.

NOTE: Pump refers to your compatible Medtronic device.

CONNECT TO PUMP ❓
Enter this Meter ID
into your Pump:
123456
Next
Go Back

6. STOP. Do <u>NOT</u> **press** <u>ANY</u> **buttons.**

This screen displays the meter ID (in the bottom left corner). This ID is needed to complete the connection process.

Put down your meter. Pick up the compatible Medtronic device and continue with Step 7.

MAIN MENU
Basal
Reservoir + Set
Utilities

7. Press **ACT** to go to the **MAIN MENU**. Scroll to **Utilities** by pressing the down arrow. Press **ACT**.

6

UTILITIES MENU
Alarm Clock
Connect Devices
Block

DEVICE OPTIONS
Meters
Remotes
Other Devices

8. Scroll to **Connect Devices** and press **ACT**.

Then scroll to **Meters** and press **ACT**.

NOTE: If your UTILITIES MENU does not contain Connect Devices, scroll to Meter Options and press ACT.

METER OPTION
Off
On

9. Select **On** and press **ACT**. If you are **replacing** a meter, go to **Step 10**. If you are **adding** a new meter, go to **Step 12**.

METER ID MENU
Add ID
Delete ID
Review ID

10. To replace a meter, select **Delete ID** and press **ACT**.

DELETE METER ID
1. aaaaaa
2. bbbbbb
3. ------

11. If you have multiple meter IDs, repeat Step 10 for each one.

METER ID MENU
Add ID
Delete ID
Review ID

ADD METER ID

1 2 3 4 5 6

12. To add a new meter, select **Add ID** and press **ACT**. Refer to Step 6 (or see meter back) to find meter ID (SN).

Use the up and down arrow buttons to enter the six character meter ID shown on the meter screen.

Press **ACT** after each character entry.

SN
123456

7

METER ID MENU
Add ID
Delete ID
Review ID

13. Select Review ID on your compatible Medtronic device to confirm that your CONTOUR®NEXT LINK meter ID has been correctly entered. If incorrect, go back to Step 10.

REVIEW METER ID
1. 123456
2. ------
3. ------

NOTE: For detailed instructions, see your compatible Medtronic device user guide.

CONNECT TO PUMP
Enter this Meter ID into your pump:
123456   Next
              Go Back

14. Return to your CONTOUR NEXT LINK meter. After you have entered the meter ID into your compatible Medtronic device, press Next.

Meter Send Options

15. After the meter and pump are connected, you will need to set your **Send Options**. This controls how your meter sends blood glucose readings to your Medtronic pump.

Your options are:

Always	Meter will always send results
Ask Me	Meter will ask you before sending results
Never	Meter will never send results

SEND OPTIONS
Automatically send results to the Pump?   Always
                                               Ask me
                                               Never

Press the **Send Option** that is best for you.

Your choice can be changed later using Setup (see page 42).

✔ Send Options set. Meter will ask you before sending results.   OK

16. Press OK.

Set Date and Time to Match Medtronic Device

12:00
STATUS   0100
Battery: Normal
Mon 11 OCT 2010
S/N# 454056

CURRENT DATE & TIME
11.10.10   Accept
12:00   Change

17. The date and time on your **meter** must match the date and time on your **Medtronic device**. Pick up Medtronic device. Press **ACT** to go to the MAIN MENU. Scroll to Utilities and press **ACT**. Scroll to Time/

Date and press **ACT**. Select a time format and press **ACT**. Note the time and date.
Return to your **meter**. Follow instructions on your meter to change the time and date to match your **Medtronic device**.

AutoLog

The AutoLog feature lets you mark your test result as

⚪ Fasting	🍴 Before Meal	🍴 After Meal	No Mark

Your meter comes preset with AutoLog turned OFF.

AUTOLOG   ❓
AutoLog is Off.   Accept
                         Turn On

18. When the AutoLog screen appears, press Accept to keep AutoLog OFF. Or, to activate AutoLog, select Turn On.

High and Low Alerts

The High and Low Alert feature tells you when your test result is above or below the settings you choose. Results above High are marked High Blood Sugar. Results below Low are marked Low Blood Sugar. Alerts appear as large orange numbers.

NOTE: Alerts can only be set outside your selected Target Range(s). For additional information, please contact Diabetes Support. Contact information for Diabetes Support is on the back cover.

⚠ **WARNING**

Talk to your health care professional before setting any High or Low Alerts on your meter.

Your meter comes preset with a high alert level of 13.9 mmol/L and a low alert level of 3.9 mmol/L. You can Accept or Change these levels.

19. Select Accept to keep the preset alert levels. If you wish to change these alert levels, press Change.

NOTE: Your Target ranges must be within your High and Low Alert levels. You set your Target ranges next.

20. If you selected Change, press the ▲ or ▼ button to select your High Alert level. This can be set between 7.0 - 20.0 mmol/L. Press OK.

21. Press the ▲ or ▼ button to select your Low Alert level. This can be set between 3.0 - 5.5 mmol/L. Press OK.

NOTE: Press and hold the ▲ or ▼ button to scroll through the numbers faster.

22. The next screen confirms your choices. Press Accept to confirm your Alert settings.

Target Ranges

Next you are asked to accept your blood sugar Targets. Targets are your personal ranges for your blood sugar results. With AutoLog OFF, you have a single Target range. With AutoLog ON, you have Target ranges for Fasting, Before Meal and After Meal.

NOTE: Targets can only be set inside your selected Alert level(s). For additional information, please contact Diabetes Support. Contact information for Diabetes Support is on the back cover.

⚠ **WARNING**

Talk to your health care professional before setting any Target ranges on your meter.

23. If AutoLog is OFF, Accept or Change the preset blood sugar Target range. The preset range is 3.9 - 10.0 mmol/L.

TARGET
Fasting:
○ 3.9 – 7.2
Accept
Change

If AutoLog is ON, **Accept** or **Change** the preset blood sugar range for Fasting, Before Meal and After Meal screens. Each Target has an option to **Accept** or **Change**.

The preset values based on ADA recommendations are:[6]

○	Fasting	3.9 - 7.2 mmol/L
	Before Meal	3.9 - 7.2 mmol/L
	After Meal	3.9 - 10.0 mmol/L

TARGET
4.2 – 10.0
OK

24. To change the Targets press the ▲ or ▼ button until the desired Target is reached and then press **OK**. Press **Accept** on confirmation screen.

You can change these settings later by going to the Main Menu and selecting Setup. See page 49.

✔ Setup is complete. Insert strip to start a test.

Initial Setup is complete. You may now test your blood sugar. See Testing, below.

Testing

Getting Ready to Test
ℹ Read your CONTOUR®NEXT LINK user guide, your Medtronic device user guide, the MICROLET®2 lancing device insert and all instructional materials provided in your meter kit before testing. Please follow all instructions for use and care exactly as described.

12 Contour next link

Examine product for missing, damaged or broken parts. If the test strip bottle is open inside a new box of strips, do not use those strips. Contact Bayer Diabetes Support for replacement items. Please see back cover for contact information.

CAUTION: Your CONTOUR®NEXT LINK meter only works with CONTOUR®NEXT test strips and CONTOUR®NEXT control solutions.

Make sure you have all the materials you need ready before you begin testing. This includes your CONTOUR NEXT LINK meter, CONTOUR NEXT test strips and the MICROLET®2 lancing device and MICROLET® lancets. You may also need CONTOUR NEXT control solution to perform a quality control check. CONTOUR NEXT control solutions are available separately if not included in the meter kit.
- Do not perform a blood glucose test when your meter is connected to an external device, e.g., computer.
- Use only approved cables or wall charger from the manufacturer or a 5V charger that displays a CE mark.

Preparing the Lancing Device

⚠ **WARNING: Potential Biohazard**
The MICROLET 2 lancing device is intended for self-testing by a single patient. It must not be used on more than one person due to the risk of infection.

⊗ Use a new MICROLET lancet each time you test because it is no longer sterile after use.

Read the MICROLET 2 lancing device insert for complete instructions. If you are using a different lancing device, see that manufacturer's instructions for use. For Alternative Site Testing instructions, see page 19.

1. Remove the endcap from the MICROLET 2 lancing device with your thumb on the grip indent as shown. Snap the endcap off from top to bottom.

13

2. Loosen the round protective cap on the lancet by rotating it ¼ turn, but do not remove it. Always use MICROLET® lancets for the best operation.

3. Insert the lancet firmly into the lancing device until it comes to a full stop. This will set the device. You can also pull and release the re-setting handle.

4. Twist off the round protective lancet cap. Save it for disposing of the used lancet.

5. Replace the grey endcap before getting blood drop.

6. The puncture depth depends on the endcap setting and the amount of pressure applied to the puncture site. Rotate the endcap dial to adjust the puncture depth.

Preparing the Test Strip

⚠️ **WARNING**

Always wash your hands with soap and water and dry them well before and after testing, handling the meter, lancing device or test strips.

14

1. Remove a CONTOUR®NEXT test strip from the bottle. **Tightly close the bottle lid immediately after you have removed the test strip.**

2. Hold the test strip with the grey square end facing up.

3. Insert the grey square end into the test strip port until the meter beeps (if the Sound is set to ON).

You will see the **Apply Blood** screen. The meter is now ready for you to test.

NOTE: After test strip is inserted, if you do not apply blood to the test strip within 1 minute, the meter screen will dim and the meter will beep. Press any button and the Apply Blood screen will become bright again. After a total of 3 minutes of inactivity the meter will turn off.

Getting the Blood Drop — Fingertip Testing

1. Press the endcap firmly against the puncture site and press the blue release button with your thumb.

2. Stroke your hand and finger toward the puncture site to form a drop of blood. Do not squeeze around the puncture site.

15

3. Test immediately after a good drop of blood has formed.

4. Immediately touch the tip of the test strip to the drop of blood. The blood is pulled into the test strip through the tip.

Hold the tip of the test strip in the blood drop until the meter beeps.

Do not press the tip against the skin or place the blood on top of the test strip or you could get inaccurate results or errors.

Apply More Blood

STRIP UNDERFILLED

APPLY MORE BLOOD NOW

If the first blood drop is not enough, the meter will beep twice and display "**STRIP UNDERFILLED**" and "**APPLY MORE BLOOD NOW**." You have about 30 seconds to apply more blood to the same strip.

! Too Little Blood
Remove used strip. Repeat test with new strip.
E01

If you do not re-apply enough blood within about 30 seconds, you will see a screen telling you to remove the strip and repeat with a new strip.

16

Test Results

Testing With AutoLog Off

TESTING...
5

9.3

After applying blood to the test strip when AutoLog is turned OFF, your result will appear after the 5 second countdown.

YOUR RESULTS ❓
9.3 mmol L
Send
Don't Send

If **Always** was selected in Send Options during Setup, your result is automatically sent to your pump. If **Never** was selected in Send

Options, you will not have the option to send the result to your pump. If **Ask Me** was selected in Send Options, you can choose to send your result to your pump after each blood sugar test. Press **Send** or **Don't Send**. If **Send** is chosen, press **OK** on the Send confirmation screen.

Leave the test strip in the meter to set an optional reminder for your next test (see page 31) or add a note (see page 34).

10:30 | 11.10
9.3 mmol L
Reminder
Sent
Notes

If you have completed your test, remove the test strip from the meter. Press and hold the top **Menu** button to turn off the meter. The meter also turns off after 3 minutes of inactivity.

CAUTION: Always check the display on your pump to ensure that the glucose result shown agrees with the glucose result shown on the meter.

17

Testing With AutoLog On

After you apply blood to the test strip, use the ▼ to select **Fasting**, **Before Meal**, **After Meal** or **No Mark**, and then press **OK**. (Scroll down to see **No Mark**.)

NOTE:
- **Your test result does not display until you make an AutoLog selection.**
- **If your result is above or below your High or Low Alert settings, you will see your result without pushing a button.**

◯ Fasting	The Fasting marker can be used when testing blood sugar levels after going without food and sugared drink for 8 hours.
🍎 Before Meal	The Before Meal marker can be used when testing blood sugar levels within 1 hour before a meal.
🍴 After Meal	The After Meal marker can be used when testing blood sugar levels within 2 hours after a meal.
No Mark	You can select **No Mark** if you are testing at times other than before or after a meal or fasting.

If you make your AutoLog selection very quickly, you may see the remainder of the testing countdown.

Your test result appears as a large number and then changes to the usual test result screen.

18

If **Always** was selected in Send Options during Setup, your result is automatically sent to your pump. If **Never** was selected in Send Options, you will not have the option to send the result to your pump. If **Ask Me** was selected in Send Options, you can choose to send your result to your pump after each blood sugar test. Press **Send** or **Don't Send**. If **Send** is chosen, press **OK** on the Send confirmation screen.

Leave the test strip in the meter to set a reminder for your next test (see page 31) or add a note (see page 34).

If you have completed your test, remove the test strip. To turn off the meter, press and hold the top **Menu** button. Or, after 3 minutes of inactivity, the meter turns off automatically.

CAUTION: Always check the display on your pump to ensure that the glucose result shown agrees with the glucose result shown on the meter.

Alternative Site Testing (AST) — Palm

⚠️ **WARNING**
- **Ask your health care professional if Alternative Site Testing is right for you.**
- **Do not calibrate your continuous glucose monitoring device from an AST result.**
- **Do not calculate a bolus based on an AST result.**

IMPORTANT: For Alternative Site Testing, use the clear endcap on your lancing device. Your CONTOUR®NEXT LINK meter can be used for fingertip or palm testing. See the MICROLET®2 insert for complete instructions for Alternative Site Testing.

19

IMPORTANT: Do not use AST under the following conditions:

• If you think your blood sugar is low
• When blood sugar is changing rapidly (after a meal, insulin dose or exercise)
• If you are unable to feel symptoms of low blood sugar (hypoglycaemic unawareness)
• If you get alternative site blood sugar results that do not agree with how you feel
• During illness or times of stress
• If you will be driving a car or operating machinery

Alternative Site test results may be different from fingertip results when glucose levels are changing rapidly (e.g., after a meal, after taking insulin or during or after exercise). Additionally, glucose levels may not rise as high or fall as low as levels in the fingertip. As such, fingertip testing results may identify hypoglycaemic levels sooner than alternate site results.

Alternative Site Testing is recommended only when it is more than 2 hours after a meal, diabetes medication or exercise.

If you do not have a clear endcap to perform AST, contact Bayer Diabetes Support. Please see back cover for contact information.

Getting a Blood Drop for Alternative Site Testing

1. Wash your hands and the puncture site with soap and warm water. Rinse and dry well.

2. Attach the clear AST endcap to the MICROLET®2 lancing device.

3. Select a puncture site from a fleshy area on the palm. Avoid veins, moles, bones and tendons.

4. Press the clear endcap firmly against the puncture site and then press the blue release button.

5. Maintain steady pressure until a small, round blood drop forms.

6. Lift the device straight up and away from the skin without smearing the blood.

7. Test immediately after you have formed a small, round blood drop.
Immediately touch the tip of the test strip to the drop of blood. The blood is pulled into the test strip through the tip.

Do not test the blood sample from palm if you get:

• Smeared blood
• Clotted blood
• Runny blood
• Clear fluid mixed with the blood

8. Hold the tip of the test strip in the blood drop until the meter beeps. Do not press the tip against the skin or place the blood on top of the test strip or you could get inaccurate results or errors.

STRIP UNDERFILLED

APPLY MORE BLOOD NOW

If the first blood drop is not enough, the meter will beep twice and display "**STRIP UNDERFILLED**" and "**APPLY MORE BLOOD NOW**." You have about 30 seconds to apply more blood to the same strip.

! **Too Little Blood**
Remove used strip.
Repeat test with new
E01 strip.

If you do not apply more blood within about 30 seconds, remove the strip and repeat with a new strip.

AUTOLOG
⚪ Fasting
🍎 Before Meal
🍴 After Meal
No Mark
OK

9. If you have the AutoLog feature turned ON, the AutoLog screen appears. Select ⚪ **Fasting**, 🍎 **Before Meal**, 🍴 **After Meal** or **No Mark** by pressing the **OK** button when your selection is highlighted. Scroll down to see **No Mark**.

NOTE:
• **Your test result does not display until you make an AutoLog selection.**
• **If your result is above or below your High or Low Alert settings, you will see your result without pushing a button.**

YOUR RESULTS ❓
9.3 mmol/L   Send
🍎 Before Meal   Don't Send

If **Always** was selected in Send Options during Setup, your result is automatically sent to your pump. If **Never** was selected in Send Options, you will not have the option to send the result to your pump. If **Ask Me** was selected in Send Options, you can choose to send your result to your pump after each blood sugar test. Press **Send** or **Don't Send**. If **Send** is chosen, press **OK** on the Send confirmation screen. You can change your send option at any time using the Setup Menu (see page 42).

22

⚠️ **WARNING**
• **Do not calculate a bolus based on an AST result.**
• **Do not calibrate your continuous glucose monitoring device from an AST.**

If you have completed your test, remove the test strip from the meter. Press and hold the top **Menu** button to turn off the meter. The meter also turns off after 3 minutes of inactivity.

Removing the Used Lancet

1. In one hand, hold the lancing device with your thumb on the grip indent, with your other hand, hold the endcap as shown and gently snap off the endcap.

2. Place the round protective lancet cap on a flat surface with the Bayer logo facing down.

3. With the used lancet still in the lancing device, push the lancet needle completely into the middle of the exposed side of the cap.

4. While pressing the release button (**a**), pull the re-setting handle (**b**), and the lancet will drop into the container you have selected.

⚠️ **WARNING**
• **Dispose of the used lancet as medical waste or as advised by your health care professional.**
• ⊗ **Do not reuse lancets. Use a new MICROLET® lancet each time you test.**

23

> **⚠ WARNING: Potential Biohazard**
> - Always dispose of test strip and lancet as medical waste or as advised by your health care professional. All products that come in contact with human blood should be handled as if capable of transmitting infectious diseases.
> - Please refer to your MICROLET®2 package insert for instructions on how to properly remove and dispose of the lancet.

Test Results — Expected Values

Blood glucose values will vary depending on food intake, medication dosages, health, stress or activity. Non diabetic plasma glucose concentrations are normally maintained within a relatively narrow range, approximately 3.9 - 6.1 mmol/L in a fasting state.[7]

> **⚠ WARNING**
> You should consult your health care professional for glucose values specific to your needs.
> - If your blood sugar reading is under 2.8 mmol/L, follow medical advice immediately.
> - If your blood sugar reading is over 13.9 mmol/L, wash and dry your hands well and repeat the test with a new strip. If you get a similar result, follow medical advice immediately.
> - Always consult your health care professional before changing your medication based on test results.

High and Low Blood Sugar Alert Screens

Your meter has been preset with a low blood sugar (hypoglycaemia) value of 3.9 mmol/L and a high blood sugar (hyperglycaemia) value of 13.9 mmol/L. These are the preset values, but can be customized by you and/or your health care professional. You can change the High and Low Alert levels under Main Menu, Setup option (see page 52).

If your blood sugar reading is under your low blood sugar alert level:

3.8
Low Blood Sugar

- A screen with large orange numbers alerts you that your blood sugar is low.

If your blood sugar reading is over your high blood sugar alert level:

14.0
High Blood Sugar

- A screen with large orange numbers alerts you that your blood sugar is high.

- If AutoLog is ON and you did not mark your result before the high or low alert appeared, select **Notes**.

- Press the ▲ or ▼ button to scroll through the choices.
- Press **OK** when your choice is highlighted.

NOTE: If the highlight is over an item that has previously been selected, you will see a red "X" instead of "OK."

Testing in the Dark

Your meter has a lighted test strip port to help you test in the dark.

- With the meter off, give the top **Menu** button two quick presses to turn on the test strip port light.
- Insert a test strip and the display screen appears.
- Once blood is applied to the test strip, the light goes off.
- Continue with your test.
- Two quick presses of the top **Menu** button also turns off the light.

Control Solution Testing

<div>

⚠ **WARNING**
Shake the control solution well before testing.

</div>

CAUTION: Use only CONTOUR®NEXT control solution from Bayer with your CONTOUR®NEXT LINK blood glucose monitoring system. Using anything other than CONTOUR NEXT control solution can cause inaccurate results.

Quality Control

You should perform a control test when:
- using your meter for the first time
- you open a new bottle or package of test strips
- you think your meter may not be working correctly
- you have repeated, unexpected blood glucose results

<div>

⚠ **WARNING**
• **Do not calibrate your continuous glucose monitoring device from a control result.**
• **Do not calculate a bolus based on a control result.**

</div>

CAUTION: Check the expiry date on the test strip bottle and the expiry date and discard date on the control solution bottle. DO NOT use expired materials.

Control solutions are available separately if not included in the meter kit. Always use CONTOUR NEXT control solutions from Bayer. Other brands could present incorrect results. If you need help locating CONTOUR NEXT control solutions from Bayer, contact Bayer Diabetes Support. Please see back cover for contact information.

1. Remove the test strip from the bottle and firmly snap the lid closed.

2. Hold the test strip with the grey square end facing up.

3. Insert the grey square end of the test strip into the test strip port until the meter beeps.

4. You will see the **Apply Blood** screen. The meter is now ready for you to test.

5. Shake the control solution bottle well before every use.

6. Remove bottle cap and use a tissue to wipe away any solution around the bottle tip before dispensing a drop.

7. Squeeze a small drop of control solution on a clean non-absorbent surface.

Do not apply control solution to your finger or to the test strip directly from the bottle.

8. Immediately touch the tip of the test strip to the drop of control solution.

9. **Hold the tip in the drop until the meter beeps.**

10. The meter shows the AutoLog screen (if AutoLog is ON) but will sense control solution. The meter will count down for 5 seconds and the control test result will display on the meter. It automatically marks the result as a "Control Test" and stores it in the memory. Control test results are not included in your blood sugar averages.

11. Compare your control test result to the ranges printed on the test strip bottle.

12. Remove test strip. To turn the meter off, press and hold the **Menu** button, OR, after 3 minutes of inactivity, the meter turns off. Dispose of the used test strip as medical waste or as advised by your health care professional.

NOTE: Control test results that are marked as "Control Test" are not transmitted to the pump.

⚠️ **WARNING**
- **If the control solution test result is out of range, the result may be transmitted to your pump when in "Always" send mode (see page 30).**
- **Do not send an out of range control result to your pump.**

CAUTION: If your control solution test result is out of range, contact Bayer Diabetes Support. Please see back cover for contact information. Do not use the meter or test strips for blood glucose testing until the issue is resolved.

Features

Your CONTOUR®NEXT LINK meter includes many testing features.

AutoLog (Marking Your Results)

Your meter comes with an AutoLog feature that lets you mark your test result as ○ Fasting, 🍎 Before Meal, 🍴 After Meal and No Mark.

Your meter comes with AutoLog OFF. If you would like to see your results when Fasting, Before Meal or After Meal, we recommend that you turn on this feature (see page 47).

If you have turned AutoLog ON in Setup, before your test result is displayed, the AutoLog screen appears. However, if your result is above your High Alert setting or below your Low Alert setting, you will always see your result in 5 seconds without pressing a button.

Sending Results to Your Pump

You can send your results to the pump during testing. During Initial Setup (Send Options) or in Setup (Pump Options - Send Options), choose **Ask Me** or **Always**.

If **Always** was selected in Send Options during Setup, your result is automatically sent to your pump. If **Never** was selected in Send Options, you will not have the option to send the result to your pump. If **Ask Me** was selected in Send Options, you can choose to send your result to your pump after each blood sugar test.

Press **Send** or **Don't Send**. You can change your Send Option at any time using the Setup Menu (see page 42).

CAUTION:
- You may want to test with Send Options set to Never if you do not want to create a wireless signal (for example, if you have been asked to turn off all electronic devices in an aircraft).
- Always check the display on your pump to ensure that the glucose result shown agrees with the meter display.

Test Reminders

A reminder for your next test can be set after testing OR from the Setup Menu (see page 43).

A reminder can be set in 15-minute increments from 15 minutes to 23 hours, 45 minutes.

Setting a Test Reminder
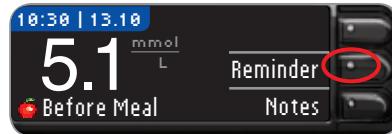
1. With the test strip still in the meter, press **Reminder**.

OR from the Setup Menu press the ▼ button to highlight **Reminder: Off**. Press **OK** to turn the Reminder ON.

2. Press **Start** to begin the countdown. The preset time is 2 hours or, if you have changed it, the last reminder time that you set is now the default.

You can change the Reminder Countdown time by pressing **Change**.

Turning Off a Test Reminder

A reminder can be turned off or changed after testing or from the Setup Menu.

NOTE: If you do a blood sugar test within 15 minutes of a set reminder, the reminder turns off automatically.

1. Press **Reminder**. If the countdown is currently on, the screen will read "**Reminder In**" with the remaining amount of time displayed.

2. To stop the countdown, press **Stop**.

A confirmation screen appears and the countdown stops.

Changing a Reminder Time

1. Press the ▲ or ▼ button to select the correct hours and minutes (in 15-minute increments).

2. Press **OK** after each selection.

A screen confirms the reminder countdown time.

When the Reminder feature is on, the clock symbol appears in the headers on the Setup and Main Menu screens.

The meter retains the reminder time that you set until you change it or turn it off.

Getting a Reminder

When the reminder time is reached, 20 beeps will sound. The meter will turn on and a reminder screen will appear.

You can stop the beeps in two ways:

1. Press **OK**, insert a test strip and proceed with testing, OR

2. Insert a test strip and proceed with testing (see page 12).

NOTE: If you decide to test within 15 minutes before the reminder time, the countdown is stopped with the insertion of the test strip. Proceed with testing.

Notes

You may add notes to your test result that may help explain results. Your notes will be saved in the Logbook. The option to add a note is available only after a test result.

1. From the test result screen, press **Notes**.

ADD NOTES
- Fasting
- Before Meal `OK`
- After Meal
- Time After Meal
- Don't Feel Right
- Sick

2. Press the ▲ or ▼ button to scroll through the choices. Some may not be visible until you scroll down. Press **OK** when your choice is highlighted.

A screen confirms your choice.

NOTE:

ADD NOTES
- Before Meal
- ✔ After Meal `✕`
- Time After Meal
- Don't Feel Right
- Sick
- Stress
- Activity
- Go Back

- **If the highlight is over an item that has previously been selected, you will see a red "X" instead of "OK."**
- **When you choose After Meal, Time After Meal will become selectable. Select Time After Meal and then you can select times from 15 minutes to 3 hours.**

After the confirmation screen disappears, you may remove the note or add one or more notes by repeating the steps above. The notes will scroll across the bottom so that you can read them all. While you can add more than one note, only one AutoLog option can be chosen (e.g., Fasting, Before Meal or After Meal).

Using the Main Menu

The Main Menu has three choices: Logbook, Trends and Setup. Select one by pressing the button next to your choice.

menu
- Logbook
- Trends
- Setup

Logbook

The Logbook contains blood sugar test results and notes that you have made to those test results. The Logbook will hold up to 1,000 results. When the maximum is reached, the oldest test result will be removed as a new test is completed and saved to the Logbook. A sound indicates the last entry.

1. To review entries in the Logbook, press and hold the top **Menu** button to turn the meter on.

2. Press the button next to **Logbook**.

LOGBOOK
9.3 mmol/L   06.11.09 10:30
Sent, Before Meal ▼

3. You can scroll through all your stored test results using the ▼ button.

END OF LOGBOOK
5.4 mmol/L   05.11.09 11:24
Sent, After Meal

When you reach the oldest entry you will see the End of Logbook screen.

Trends (Averages and Summaries)

The Trends feature displays your averages and your results as they compare to your Targets, over a period of time that you select. The options available are 7, 14, 30 and 90 day averages. Your meter has been preset to 14 day averages, but you can change this under Trends Range in the Setup Menu (see page 51).

Your 90 day average is not intended to be reflective of your HbA1c result.

Your screen will display the total number of test results included in the average and the number of tests above ⬆, within ✔ and below ⬇ Target.

Viewing Trends With AutoLog Off

Your meter has been preset to 14 day averages. You can change the Trends time range to 7, 30 or 90 days in Setup.

1. Press and hold the top **Menu** button to turn the meter on.
2. Press the button next to Trends.

TRENDS

TARGET: 3.9 – 7.2

14 DAY RESULTS
AVERAGE
9.7 mmol L   45   ⬆ 18   ✔ 22   ⬇ 5
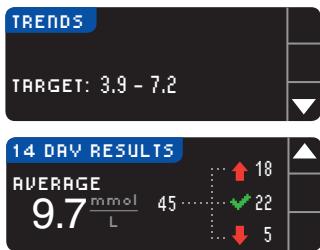
3. Press the ▼ button to display the 14 Day Results screen.

Viewing Trends With AutoLog On

1. Press and hold the top **Menu** button to turn the meter on.
2. Press the ▼ button to highlight Trends. Press OK to select.

14 DAY FASTING
AVERAGE
7.1 mmol L   60   ⬆ 12   ✔ 8   ⬇ 40

3. Press the ▼ button to display the 14 Day Fasting Average. If you have marked any test results as Fasting, you will see your Fasting Average first.

14 DAY BEFORE MEAL
AVERAGE
7.1 mmol L   38   ⬆ 8   ✔ 26   ⬇ 4

4. Press the ▼ button to go to the 14 Day Before Meal Average.

This example shows that your Before Meal average is 7.1 mmol/L and 38 test results are included in the Before Meal average with 26 within ✔ the Target range, 8 above ⬆ the Target range and 4 below ⬇ the Target range.

14 DAY AFTER MEAL
AVERAGE
9.7 mmol L   17   ⬆ 9   ✔ 8   ⬇ 0

5. Press the ▼ button to go to the 14 Day After Meal Average.

14 DAY RESULTS
AVERAGE
9.7 mmol L   Results: 115

6. Press the ▼ button to go to the 14 Day Results screen.

Setup

You can view and change options on your meter and personalize it from the Setup Menu.

1. Press and hold the top **Menu** button to turn the meter on.
2. Press the button next to **Setup**.

SETUP
- Pump Options
- Reminder
- Date
- Time
- Sound
- AutoLog
- Target
- Trends Range
- High and Low Alerts
- Language
- Customer Service
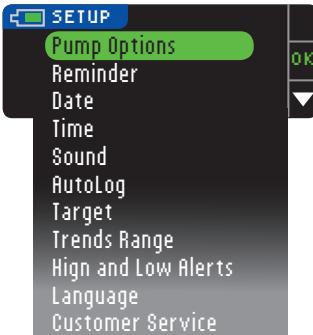
The current settings in the meter for the **Reminder**, **Date**, **Time**, **Sound** and **AutoLog** can be viewed by scrolling through the Setup Menu items. To view the settings of the other items, or to make any changes to any of the items, you can select the item using the ▲ and ▼ keys and pressing **OK**.

Pump Options

Pump Options allows you to connect to a Medtronic pump and change your Send Settings (how your blood sugar readings are sent to your pump).

Connecting the Meter and Pump

You can send blood sugar results to your pump if your meter and pump are connected.

1. Press and hold the top **Menu** button to turn the meter on.
2. Press the button next to **Setup**.

SETUP
- Pump Options
- Reminder
- Date

3. Press **OK** to select **Pump Options**.

PUMP OPTIONS
- Send Options
- Connection
- Go Back

4. Press **Connection**.

CONNECT TO PUMP
Connect to a MiniMed Pump?
- OK
- Go Back

5. Press **OK** to begin the connection process.

   NOTE: Pump refers to your compatible Medtronic device.

CONNECT TO PUMP
Enter this Meter ID into your Pump: 123456
- Next
- Go Back

6. **STOP. Do NOT press ANY buttons.**

   This screen displays the meter ID number (in the bottom left corner). This ID is needed to complete the connection process.

   Put down your meter. Pick up the compatible Medtronic device and continue with Step 7.

MAIN MENU
Basal
Reservoir + Set
Utilities

7. Press **ACT** to go to the **MAIN MENU**. Scroll to **Utilities** by pressing the down arrow. Press **ACT**.

UTILITIES MENU
Alarm Clock
Connect Devices
Block

DEVICE OPTIONS
Meters
Remotes
Other Devices

8. Scroll to **Connect Devices** and press **ACT**.

Then scroll to **Meters** and press **ACT**.

NOTE: If your UTILITIES MENU does not contain Connect Devices, scroll to Meter Options and press ACT.

METER OPTION
Off
On

9. Select **On** and press **ACT**. If you are **replacing** a meter, go to **Step 10**. If you are **adding** a new meter, go to **Step 12**.

METER ID MENU
Add ID
Delete ID
Review ID

10. To replace a meter, select **Delete ID** and press **ACT**.

DELETE METER ID
1. aaaaaa
2. bbbbbb
3. ------

11. If you have multiple meter IDs, repeat Step 10 for each one.

METER ID MENU
Add ID
Delete ID
Review ID

ADD METER ID

1 2 3 4 5 6

12. To add a new meter, select **Add ID** and press **ACT**. Refer to Step 6 (or see meter back) to find meter ID (SN).

Use the up and down arrow buttons to enter the six character meter ID shown on the meter screen.

Press **ACT** after each character entry.

SN
123456

METER ID MENU
Add ID
Delete ID
Review ID

REVIEW METER ID
1. 123456
2. ------
3. ------

13. Select **Review ID** on your compatible Medtronic device to confirm that your CONTOUR®NEXT LINK meter ID has been correctly entered. If incorrect, go back to Step 10.

NOTE: For detailed instructions, see your compatible Medtronic device user guide.

CONNECT TO PUMP
Enter this Meter ID into your pump:
123456
Next
Go Back

14. Return to your CONTOUR NEXT LINK meter. After you have entered the meter ID into your compatible Medtronic device, press **Next**.

15. After the meter and pump are connected, you set your **Send Options**. This controls how your meter sends blood glucose readings to your Medtronic pump. Choose the **Send Option** that is best for you.

Your options are:

Always	Meter will always send results
Ask Me	Meter will ask you before sending results
Never	Meter will never send results

SEND OPTIONS
Automatically send results to the Pump?
Always
Ask me
Never

16. The next screen confirms your Send Option choice. Press **OK**.

Send Options set. Meter will ask you before sending results. OK

NOTE: If you want to disconnect the pump from the meter, you do not need to take action on your meter. Please refer to your Medtronic device user guide.

Changing the Send Option

Send Options control how your meter sends your test results to your pump. You have 3 choices:

Always	Meter will always send results
Ask Me	Meter will ask you before sending results
Never	Meter will never send results

NOTE: You may want to test with the Send Option set to Never if you do not want to create a wireless signal (for example, if you have been asked to turn off all electronic devices on an aircraft).

1. Press and hold the top **Menu** button to turn the meter on.

2. Press the button next to **Setup**.

SETUP
Pump Options
Reminder
Date

3. Press the ▼ button to highlight **Pump Options**. Press **OK** to select.

PUMP OPTIONS
Send Options
Connection
Go Back

4. Press **Send Options**.

NOTE: For Connection settings, see page 38.

SEND OPTIONS
Send is set to Always.
Change
Go Back

5. To change the current Send Option, press **Change**.

SEND OPTIONS
Automatically send results to the Pump?
Always
Ask me
Never

6. Choose the Send Option that is best for you.

Send Options set. Meter will ask you before sending results. OK

7. A confirmation screen appears. Press **OK** to return to Pump Options.

Test Reminders

A reminder for your next test can be set after testing or from the Setup Menu. See page 31 for Setting a Test Reminder after Testing.

Setting a Reminder

1. Press and hold the top **Menu** button to turn the meter on.

2. Press the button next to **Setup**.

SETUP
Pump Options
Reminder: Off
Date

3. Press the ▼ button to highlight **Reminder: Off**. Press **OK** to turn ON the reminder.

REMINDER
COUNTDOWN
2 hrs   00 mins
Start
Change
Go Back

4. To accept the preset time shown, select **Start**. To change the time, select **Change**. Use the ▲ and ▼ buttons to change the reminder time in 15-minute increments from 15 minutes to 23 hours, 45 minutes.

Contour next link

5. After you have selected hours, press **OK**. After you have selected minutes, press **OK**.

REMINDER
CHANGE COUNTDOWN
OK
3 hrs 15 mins

6. A confirmation screen appears and you can select **Change** or **Done**.

Reminder in:
3 hrs 15 mins   Change
Done

If you accept the reminder, a reminder icon ⏱ will appear in the Setup and Main Menu headers.

NOTE: If you decide to test within 15 minutes before the reminder time, the countdown stops when you insert a test strip.

Turning Off a Reminder

To turn off a reminder, you can use the Setup Menu or do a blood sugar test within 15 minutes of the reminder time. To use the Setup Menu:

1. Press and hold the top **Menu** button to turn the meter on.

2. Press the button next to **Setup**.

⏱ SETUP
Pump Options
Reminder: On
Date
OK

3. Press the ▼ button to highlight **Reminder: On**. Press **OK** to turn the Reminder OFF.

REMINDER
REMINDER IN   Stop
2 hrs 30 mins   Change
Go Back

4. Select **Stop**. A confirmation screen appears and the countdown stops.

SETUP
Pump Options
Reminder: Off
Date
OK

5. Reminder is now off.

Date and Time
Setting or Changing the Date

1. Press and hold the top **Menu** button to turn the meter on.

2. Press the button next to **Setup**.

SETUP
Reminder
Date: 13.10.10
Time
OK

3. Press the ▼ button to highlight **Date**. Press **OK** to select.

DATE
dd.mm.yy   Change
13.10.10   Go Back

4. To change the date, press **Change**.

DATE
SELECT   Month/Day/Year
Day.Month.Year

5. Select either format, **Month/Day/Year** or **Day.Month.Year**.

DATE
CHANGE YEAR
13.10.11
OK

6. Press the ▲ or ▼ button to select the correct year, month and day. Press **OK** after each selection.

✔ Date is set.
13.10.11   Done
Change

7. A screen confirms the date you entered. Press **Done** if the date is correct.

Contour next link

Setting or Changing the Time

1. Press and hold the top **Menu** button to turn the meter on.
2. Press the button next to **Setup**.

SETUP	
Date	OK
Time: 11:30	
Sound	▼

3. Press the ▼ button to highlight **Time**. Press **OK** to select.

TIME	
24 HOUR CLOCK	Change
11:30	Go Back

4. To change the time, press **Change**.

TIME	
SELECT	
	12 Hour Clock
	24 Hour Clock

5. Select either the **12 Hour Clock** or **24 Hour Clock** option.

TIME	
CHANGE HOURS	
10:30 AM	OK

6. Press the ▲ or ▼ button to select the correct hour and minute. Press **OK** after each selection.

7. If you have selected the 12 hour clock format, press the ▲ or ▼ button to select **AM** or **PM**.

✔ Time is set.	
10:30	Done
	Change

8. Time is set. A screen confirms your choice. Press **Done**.

Sound

Turning the Sound On/Off

Sound is ON when you receive your meter. Some error messages and the Reminder bell will override the Sound Off setting.

1. Press and hold the top **Menu** button to turn the meter on.
2. Press the button next to **Setup**.

SETUP	
Time	OK
Sound: On	
AutoLog	▼

3. Press the ▼ button to select **Sound**. Press **OK**.

SOUND	
Sound is On.	Accept
	Turn Off

4. To turn the sound OFF, press **Turn Off**. To keep the sound turned ON, press **Accept**.

✔ Sound is Off.

A screen confirms your choice.

AutoLog

NOTE: Your meter comes with AutoLog turned OFF.

The AutoLog feature lets you mark your test result as

○ Fasting	🍎 Before Meal	🍴 After Meal	No Mark

To Turn On AutoLog

1. Press and hold the top **Menu** button to turn the meter on.
2. Press the button next to **Setup**.

SETUP
Sound
AutoLog: Off
Target

3. Press the ▼ button to highlight `AutoLog`. Press `OK` to select.

AUTOLOG
AutoLog is Off.   **Accept**
   Turn On

4. Press `Turn On` to activate AutoLog.

✔ AutoLog is On.

A screen confirms your choice.

NOTE:
- **When you change your AutoLog setting to ON, you are asked to confirm your Target settings for Fasting, Before Meal and After Meal.**
- **Your test result does not display until you make an AutoLog selection.**
- **If your result is above or below your High or Low Alert settings, you will see your result without pushing a button.**

To Turn Off AutoLog

NOTE: Your meter comes with AutoLog OFF.

1. Press and hold the top **Menu** button to turn the meter on.
2. Press the button next to `Setup`.

SETUP
Sound
AutoLog: On
Target

3. Press the ▼ button to highlight `AutoLog`. Press `OK` to select.

AUTOLOG
AutoLog is On.   **Accept**
   Turn Off

4. To turn AutoLog OFF, press `Turn Off`.

48

✔ AutoLog is Off.

A screen confirms your choice.

NOTE: When you change your AutoLog setting to OFF, you are asked to confirm your Target setting.

Blood Sugar Targets

Targets are your personal ranges for your blood sugar results. With AutoLog OFF, you have a single Target range. With AutoLog ON, you have Target ranges for Fasting, Before Meal, and After Meal.

> ⚠ **WARNING**
> **Talk to your health care professional before setting any Target ranges on your meter.**

Changing Targets With AutoLog Off

When AutoLog is OFF, you have only one Target range. It comes preset to 3.9 - 10.0 mmol/L.

NOTE: Targets can only be set inside your selected Alert level(s). For additional information, please contact Diabetes Support. Contact information for Diabetes Support is on the back cover.

1. Press and hold the top **Menu** button to turn the meter on.
2. Press the button next to `Setup`.

SETUP
AutoLog
Target
Trends Range

3. Press the ▼ button to highlight `Target`. Press `OK` to select.

TARGET
3.9 – 10.0   **Accept**
   Change

4. To make changes to your Target range, press `Change`.

49

5. Use the ▲ or ▼ button to change each value of the Target. Press **OK** after each selection.

A screen confirms your choice.

Changing Targets With AutoLog On

When AutoLog is ON, your CONTOUR®NEXT LINK meter comes preset with the following Target ranges for testing:

	Fasting	3.9 - 7.2 mmol/L
	Before Meal	3.9 - 7.2 mmol/L
	After Meal	3.9 - 10.0 mmol/L

Ranges can be changed to personal Targets decided by you and/or your health care professional.

NOTE: Targets can only be set inside your selected Alert level(s). For additional information, please contact Diabetes Support. Contact information for Diabetes Support is on the back cover.

1. Press and hold the top **Menu** button to turn the meter on.
2. Press the button next to **Setup**.

**3.** Press the ▼ button to highlight **Target**. Press **OK** to select.

4. To make changes to your Fasting Target range, press **Change**, otherwise press **Accept**.

50

5. Press the ▲ or ▼ button to select your desired Fasting Targets. Press **OK** after each selection.

6. Repeat this process to set your personal Before Meal Targets and After Meal Targets.
7. Press **OK** after each selection.

A screen confirms that all Target ranges are set.

If correct, press **Done** to return to the Setup Menu.
To make changes, press **Change** and repeat the process.

Trends Range

The Trends feature displays your averages and your results as they compare to your Targets, over a period of time that you select. The options available are 7, 14, 30 and 90 day averages. Your meter has been preset to 14 day averages, but you can change this in Setup.

1. Press and hold the top **Menu** button to turn the meter on.
2. Press the button next to **Setup**.

3. Press the ▼ button to highlight **Trends Range**.
4. Press **OK** to select.

5. Your current setting is displayed. You can **Accept** or **Change** your current setting.

NOTE: Your 90 day average is not intended to be reflective of your HbA1c result.

51

TRENDS RANGE

7 Day
14 Day
30 Day
90 Day

OK
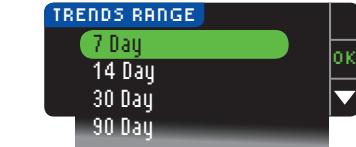
6. Select 7, 14, 30 or 90 Day by using the ▼ button and then press **OK**.

A screen confirms your choice.

High and Low Alerts

The High and Low Alerts tell you that your test result is above or below the setting you choose. Alerts appear as large orange numbers. Results above High are marked High Blood Sugar. Results below Low are marked Low Blood Sugar.

NOTE: Alerts can only be set outside your selected Target Range(s). For additional information, please contact Diabetes Support. Contact information for Diabetes Support is on the back cover.

⚠️ WARNING

Talk to your health care professional before setting any High or Low Alerts on your meter.

1. Press and hold the top **Menu** button to turn the meter on.
2. Press the button next to **Setup**.

SETUP

Trends Range
High and Low Alerts
Language

OK

3. Press the ▼ button to highlight **High and Low Alerts**. Press **OK** to select.

HIGH AND LOW ALERTS ❓

High: 13.9 mmol/L   Accept
Low: 3.9 mmol/L   Change

4. Choose **Accept** to use the preset Alert levels (or the Alert levels you chose during initial setup) for High and Low Alerts. The preset High Alert is 13.9 mmol/L and the preset Low Alert is 3.9 mmol/L.

5. Choose **Change** if you wish to use different Alert levels.

HIGH AND LOW ALERTS

High: 13.9 mmol/L   **OK**
Low: 3.9 mmol/L

6. Press the ▲ or ▼ button to select your High and Low Alert. Press **OK** after each selection.

✔️ **Alerts are set.**

High: 13.9 mmol/L   Done
Low: 3.8 mmol/L   Change

7. The next screen confirms your choices. Press **Done**.

Set Language

1. Press and hold the top **Menu** button to turn the meter on.
2. Press the button next to **Setup**.

SETUP

High and Low Alerts
Language
Customer Service

OK

3. Press the ▼ button to highlight **Language**. Press **OK** to select.

LANGUAGE

✔️ English
Hrvatski
Dansk

OK

4. Press the ▲ or ▼ button to select the language you prefer. Press ▼ to see more choices. Press **OK**.

✔️ **Language: English**

✔ OK
✖ No

5. Verify that the language you selected is displayed. Press **OK** to confirm.

If the correct language is not displayed, press **No**.

Customer Service

This option is to be used if you are speaking to a Bayer Diabetes Support representative. They will give you a code that enables them to verify certain settings. It is not for use any other time. Please see back cover for contact information.

52

53

Technical Information and Care

Transferring Data to Medtronic's CareLink Personal Therapy Management Software

You can easily transfer blood glucose results from your meter to CareLink Personal Therapy Management software.

You can also wirelessly transfer data from your compatible pump to CareLink Personal Therapy Management software using your CONTOUR®NEXT LINK meter.

1. Refer to the CareLink Personal Therapy Management software user guide for instructions on how to set up CareLink and load the required drivers onto your computer.

2. If you are running GLUCOFACTS® DELUXE diabetes management software from Bayer on your computer, you must close it.

3. Start up CareLink Personal. Follow the instructions to plug your CONTOUR NEXT LINK meter into a USB port on your computer. CareLink Personal will automatically find the CONTOUR NEXT LINK meter and your compatible pump.

Your CONTOUR NEXT LINK meter is also compatible with GLUCOFACTS DELUXE diabetes management software from Bayer, which may not be available in all countries.

> **IMPORTANT:** Your CONTOUR NEXT LINK meter from Bayer has only been tested for use with Medtronic's CareLink Personal Therapy Management software and GLUCOFACTS DELUXE diabetes management software from Bayer. Bayer is not responsible for any erroneous results from the use of other software.

For more information, contact Bayer Diabetes Support. Please see back cover for contact information.

54

Error Detection Displays

• An error screen will always have an "**E**" with a number in the lower left corner of the display.

> ⚠ **Wrong Strip Inserted**
> Repeat test with
> correct Bayer strip.
>
> E04

• If there is an error (hardware, software, testing errors) detected by your meter, your meter will beep twice.

• You will see specific instructions to guide you. The first line of the error screen will tell you the error. The next lines describe what you should do. When an error screen displays an **OK**, press the button next to it to continue.

• If you do not resolve the problem, contact Bayer Diabetes Support. Please see back cover for contact information.

Battery Status

Battery Status Displays

The battery status is displayed with a battery symbol ▭▭ on the Apply Blood screen and the Main Menu screen. It shows how much battery life is left.

▭▭ menu
Logbook
Trends
Setup

This screen displays full battery.

55

As the battery is used, the battery symbol on the screen gradually shows less fill colour. The colour of the battery fill turns yellow when the battery is low and then red when your battery is almost out of charge.

A series of low battery alerts tell you that the battery is low and to **Charge Soon**.

If you do not charge the battery, a display alerts you: "**Shutting Down, Battery is dead**." You must charge immediately.

Plug the meter into your wall charger or into the USB port of your computer. Make sure your computer is turned on and not in sleep, hibernate or power save mode.

The test strip port light flashes during charging and stops flashing and turns off when charging is complete. Please remove the meter and store in the wallet until you are ready to test.

Battery Charging

When you plug your meter into your wall charger or computer, it starts to charge immediately. While the battery charges, the test strip port light flashes slowly.

Press the top **Menu** button at any time to display the charging status.

Rapid Charge

If the battery is low when you plug in your meter, it will Rapid Charge for about 1 minute. You can run a blood sugar test as soon as Rapid Charge is complete and you have unplugged the meter.

Normal Charging

When Rapid Charge ends, normal charging is expected to last up to 2 hours when plugged into a high-powered USB port. When the battery is fully charged, the test strip port light turns off.

> **CAUTION:** Please be aware that USB ports in some computers and self-powered USB hubs can become much warmer than the room. If you wish to test immediately after disconnecting from your computer, please use the USB cable to protect the meter from exposure to heat created by the computer.

NOTE: If the charging status displays "Low Power Charging," your CONTOUR®NEXT LINK meter may be plugged into a low-powered USB port. Please try a different USB port on your computer. Only connect to a computer or a 5V charger that displays a CE mark.

End of Meter Life/Battery Removal

NOTE: Carry out this process only when you no longer intend to use the meter. The meter will not be functional once opened to remove the battery.
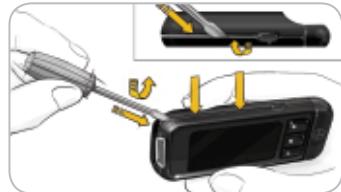
To remove the battery for proper disposal, you will need to pry the upper and lower cases apart.

With a screwdriver, beginning near the strip port, insert the tip of the screwdriver and twist to pry the case loose. Continue to do this down the side until the upper case comes apart.
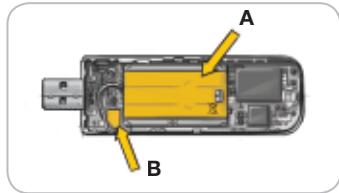
Pry up rechargeable battery here (**A**).

Disconnect battery by pulling battery connector (**B**).

Dispose of the meter and lithium polymer battery in accordance with your local/country laws and regulations.

Symptoms of High or Low Blood Sugar

You can better understand your test results by being aware of the symptoms of high or low blood sugar. Some of the most common symptoms are:

Low blood sugar (Hypoglycaemia):	High blood sugar (Hyperglycaemia):	Ketones (Ketoacidosis):
• Shakiness • Sweating • Fast Heartbeat • Blurred Vision • Confusion • Passing Out • Irritability • Seizure • Extreme Hunger • Dizziness	• Frequent Urination • Excessive Thirst • Blurred Vision • Increased Fatigue • Hunger	• Shortness of Breath • Nausea or Vomiting • Very Dry Mouth

⚠ **WARNING**

If you are experiencing any of these symptoms, test your blood sugar. If your test result is under 2.8 mmol/L or above 13.9 mmol/L, contact your health care professional immediately.

For additional information and a complete list of symptoms, contact your health care professional.

Technical Information

Accuracy

The CONTOUR®NEXT LINK blood glucose monitoring system was tested in 100 capillary blood samples using 600 CONTOUR®NEXT test strips. Two replicates were tested with 3 lots of CONTOUR NEXT test strips for a total of 600 readings. Results were compared to the YSI® glucose analyzer, which is traceable to the CDC hexokinase method.[8] The tables below compare the performance of the two methods.

Table 1 — System accuracy results for CONTOUR NEXT LINK meter using CONTOUR NEXT test strips at glucose concentration < 4.2 mmol/L

Within +/– 0.28 mmol/L	Within +/– 0.56 mmol/L	Within +/– 0.83 mmol/L
63/78 (80.8%)	78/78 (100%)	78/78 (100%)

Table 2 — System accuracy results for CONTOUR NEXT LINK meter using CONTOUR NEXT test strips at glucose concentration ≥ 4.2 mmol/L

Within +/– 5%	Within +/– 10%	Within +/– 15%	Within +/– 20%
402/522 (77.0%)	518/522 (99.2%)	522/522 (100%)	522/522 (100%)

Acceptance criteria in ISO 15197: 2003 are that 95% of all differences in glucose values (i.e., between reference method and meter) should be within +/-0.83 mmol/L for glucose values less than 4.2 mmol/L, and within +/- 20% for glucose values greater than or equal to 4.2 mmol/L.

Precision

A repeatability study was conducted with the CONTOUR®NEXT LINK blood glucose monitoring system using 5 venous whole blood specimens with glucose levels from 2.4 to 18.2 mmol/L. Multiple replicates (n=100 per lot) were tested using multiple CONTOUR NEXT LINK blood glucose meters and 3 lots of CONTOUR®NEXT test strips. The following precision results were obtained.

System repeatability results for CONTOUR NEXT LINK meter using CONTOUR NEXT test strips

Mean Glucose Level, mmol/L	Standard Deviation, mmol/L	Coefficient of Variation (%)
2.41	0.05	2.1
4.50	0.11	2.4
6.78	0.08	1.2
11.46	0.14	1.2
18.34	0.35	1.9

Principles of the Procedure

The CONTOUR NEXT LINK blood glucose test is based on measurement of electrical current caused by the reaction of the glucose with the reagents on the electrode of the strip. The blood sample is drawn into the tip of the test strip through capillary action. Glucose in the sample reacts with FAD glucose dehydrogenase (FAD-GDH) and the mediator. Electrons are generated, producing a current that is proportional to the glucose in the sample. After the reaction time, the glucose concentration in the sample is displayed. No calculation is required.

Comparison Options

The CONTOUR®NEXT LINK system is designed for use with capillary whole blood. Comparison to a laboratory method must be done simultaneously with aliquots of the same sample. Note: Glucose concentrations drop rapidly due to glycolysis (approximately 5%-7% per hour).[9]

Service Information

If you have a problem and none of the problem solving messages on the meter help, contact Bayer Diabetes Support. Please see back cover for contact information. We have trained specialists to help you.

Important

Speak to a Bayer Diabetes Support Representative before returning your meter for any reason. He/she will give you the information needed to get your problem handled correctly and efficiently.

Please have your CONTOUR®NEXT LINK blood glucose meter and CONTOUR®NEXT test strips available when you phone. It would also be helpful to have a bottle of CONTOUR®NEXT control solution suitable for your test strips nearby.

Check List

This check list may be helpful when speaking with Bayer Diabetes Support:

1. Locate the model number (**A**) and serial number (**B**) on the back of the meter.

2. Locate the test strips' expiry date on the bottle.

3. Check the battery symbol ▮▮▮ on the screen. (See page 55, Battery Status.)

Symbols Used

The following symbols are used throughout the product labeling for the CONTOUR®NEXT LINK blood glucose monitoring system (meter packaging and labeling, and reagent and control solution packaging and labeling).

Symbol	What It Means	Symbol	What It Means
	Use by date (last day of month)		Recycle Packaging
LOT	Batch code	CONT N	Control Range Normal
Discard Date:	Control Discard Date	CONT L	Control Range Low
45°C 5°C	Temperature limitations	CONT H	Control Range High
	Consult instructions for use		Do not reuse
IVD	*In Vitro* Diagnostic Medical Device	STERILE R	Sterilized using irradiation
	Manufacturer	!	Caution
REF	Catalogue number		

Symbol	What It Means
	Batteries must be disposed of in accordance with laws in your country. Contact your competent local authority for information on the relevant laws regarding disposal and recycling in your area. The meter should be treated as contaminated and disposed of according to local safety rules. It should not be disposed of with waste electronic equipment.
	The USB cable is waste electrical and electronic equipment. Do not dispose in household waste. Remember to follow local regulations.

Contact your health care professional or local waste disposal authority for medical waste disposal guidelines.

System Specifications

Test Sample: Capillary whole blood
Test Result: Referenced to plasma/serum glucose
Sample Volume: 0.6 µL
Measuring Range: 1.1 mmol/L to 33.3 mmol/L
Countdown Time: 5 seconds
Memory: Stores most recent 1,000 test results
Battery Type: Non-serviceable, 250mAh rechargeable lithium polymer battery, 3.4V – 4.2V (5V input voltage)
Meter/Battery Life: 5 years
Charging Current: 300 mA
Strip Storage Temperature Range: 30°C 0°C
Normal Control Storage Temperature Range: 30°C 9°C
Meter Operating Temperature Range: 45°C 5°C
Humidity: 10%–93% RH
Dimensions: 97 mm wide x 31 mm high x 18 mm thick
Weight: 43 grams
Sound Output: 45 to 80 dBA at a distance of 10 cm
Electromagnetic Compatibility (EMC): The CONTOUR®NEXT LINK meter complies with the electromagnetic requirements specified in ISO 15197: 2003. Electromagnetic emissions are low and unlikely to interfere with other nearby electronic equipment, nor are emissions from nearby electronic equipment likely to interfere with the CONTOUR NEXT LINK meter. Immunity to electrostatic discharge meets the requirements of IEC 61000-4-2: 2008. It is advisable to avoid use of electronic devices in very dry environments especially if synthetic materials are present. The CONTOUR NEXT LINK meter has been tested for radio frequency interference at the frequency range and test levels specified by ISO 15197: 2003. To avoid radio frequency interference, do not use the CONTOUR NEXT LINK meter near cellular or cordless telephones, walkie talkies, garage door openers, radio transmitters or other electrical or electronic equipment that are sources of electromagnetic radiation, as these may interfere with the proper operation of the meter.

Caring for Your Meter

> **CAUTION:** Avoid exposing meter and test strips to excessive humidity, heat, cold, dust or dirt.

• Store your meter in the wallet provided whenever possible.
• **Wash hands and dry well before handling to keep the meter and test strips free of water, oils and other contaminants.**
• Keep blood, control solution and cleaning fluid from entering the test strip port or USB port.
• Handle the meter carefully to avoid damaging the electronics or causing other malfunctions.
• The USB cap of your CONTOUR®NEXT LINK meter is designed to protect the USB port. Should you lose the cap, contact Bayer Diabetes Support for a replacement. Please see back cover for contact information.

Cleaning Your Meter

• The exterior of the CONTOUR NEXT LINK meter can be cleaned using a moist (not wet) lint-free tissue with a mild detergent or disinfectant solution, such as 1 part bleach mixed with 9 parts water. Wipe dry with lint-free tissue after cleaning. Do not insert anything into or attempt to clean inside the USB connection or test strip port.

> **CAUTION:** Do not allow cleaning solution to run in or around the buttons, USB cap or strip port. Doing so may cause a malfunction.

Supplies

When calling for supplies make sure you include the name of the replacement part or accessory item.

Replacement Parts
Items

• CONTOUR®NEXT LINK user guide
• CONTOUR NEXT LINK quick reference guide
• USB extension cable from Bayer
• USB cap
• Wall charger
• CONTOUR®NEXT control solution
• MICROLET®2 lancing device
• Check the website www.bayerdiabetes.com for any meter updates or GLUCOFACTS®DELUXE updates.
• To order meter items, contact Bayer Diabetes Support. Please see back cover for contact information.

References

1. Wickham NWR, Achar KN, Cove DH. Unreliability of capillary blood glucose in peripheral vascular disease. *Practical Diabetes.* 1986;3(2):100.
2. Atkin, S. et al. Fingerstick Glucose Determination in Shock. *Ann Intern Med.* 1991;114:1020-1024.
3. Desachy A, Vuagnat AC, et al. Accuracy of bedside glucometry in critically ill patients: influence of clinical characteristics and perfusion index. *Mayo Clin Proc.* 2008;83(4):400-405.
4. FDA Public Health Notification: Use of Fingerstick Devices on More than One Person Poses Risk for Transmitting Bloodborne Pathogens: Initial Communication: Update 11/29/2010. http://www.fda.gov/MedicalDevices/Safety/AlertsandNotices/ucm224025.htm
5. CDC Clinical Reminder: Use of Fingerstick Devices on More than One Person Poses Risk for Transmitting Bloodborne Pathogens (2010). http://www.cdc.gov/injectionsafety/Fingerstick-DevicesBGM.html
6. American Diabetes Association. Standards of medical care in diabetes--2012. *Diabetes Care.* 2012;35(Suppl 1):S11-63.
7. Longo D.L. et al. *Harrison's Principles of Internal Medicine,* 18th Edition, 2011. http://www.accessmedicine.com
8. Data on file, Bayer HealthCare Diabetes Care.
9. *Tietz Fundamentals of Clinical Chemistry,* 5th Edition, Edited by Burtis CA and Ashwood ER, W. B. Saunders Co., Philadelphia, PA, 2001, p. 444.

Warranty

Manufacturer's Warranty: Bayer HealthCare warrants to the original purchaser that this instrument will be free from defects in materials and workmanship for life from the date of original purchase (except as noted below). During the stated period, Bayer HealthCare shall, at no charge, replace a unit found to be defective with an equivalent or current version of the owner's model.

Limitations of Warranty: This warranty is subject to the following exceptions and limitations:

1. A 90-day warranty only will be extended for consumable parts and/or accessories.

2. This warranty is limited to replacement due to defects in parts or workmanship. Bayer HealthCare shall not be required to replace any units which malfunction or are damaged due to abuse, accidents, alteration, modification, misuse, neglect, maintenance by someone other than Bayer HealthCare or failure to operate the instrument in accordance with instructions. Further, Bayer HealthCare assumes no liability for malfunction or damage to Bayer HealthCare instruments caused by the use of reagents other than the appropriate reagents (e.g., CONTOUR®NEXT test strips) manufactured or recommended by Bayer HealthCare.

3. Bayer HealthCare reserves the right to make changes in design of this instrument without obligation to incorporate such changes into previously manufactured instruments.

4. Bayer HealthCare has no knowledge of the performance of the CONTOUR®NEXT LINK blood glucose meter when used with any test strips other than CONTOUR NEXT test strips, and therefore makes no warranty of the performance of the CONTOUR NEXT LINK meter when used with any test strips other than CONTOUR NEXT test strips or when the CONTOUR NEXT test strip is altered or modified in any manner.

5. Bayer HealthCare makes no warranty of the performance of the CONTOUR®NEXT LINK meter or test results when used with any control solution other than CONTOUR®NEXT control solution.

6. Bayer HealthCare makes no warranty of the performance of the CONTOUR NEXT LINK meter or test results when used with any software other than GLUCOFACTS® DELUXE diabetes management software from Bayer (where supported) and CareLink Personal therapy management software.

BAYER HEALTHCARE MAKES NO OTHER EXPRESS WARRANTY FOR THIS PRODUCT. THE OPTION OF REPLACEMENT, DESCRIBED ABOVE, IS BAYER HEALTHCARE'S ONLY OBLIGATION UNDER THIS WARRANTY. IN NO EVENT SHALL BAYER HEALTHCARE BE LIABLE FOR INDIRECT, SPECIAL OR CONSEQUENTIAL DAMAGES, EVEN IF BAYER HEALTHCARE HAS BEEN ADVISED OF THE POSSIBILITY OF SUCH DAMAGES.

Some jurisdictions do not allow the exclusion or limitation of incidental or consequential damages, so the above limitation or exclusion may not apply to you. This warranty gives you specific legal rights and you may also have other rights which vary from jurisdiction to jurisdiction.

For warranty service: Purchaser must contact Bayer Diabetes Support for assistance and/or instructions for the use of this instrument. Please see back cover for contact information.

Index

**Bayer Diabetes Support is available from 8:30 am - 5:30 pm
Monday - Friday on:**

0845 600 6030 - UK
www.bayerdiabetes.co.uk

1 890 920 111 – Ireland
www.bayerdiabetes.ie

CE
0088

Bayer, the Bayer Cross, CONTOUR,
GLUCOFACTS and MICROLET are
registered trademarks of Bayer. The
No Coding logo is a trademark of Bayer.

Medtronic

All other trademarks are the property of
their respective owners.

Bayer